

Description

Pro Strips™ 5 Simulation Device is designed to provide a demonstration of the type of results that can be achieved using the Pro Strips PS-5T or ATTAK kits

Important Information

Please review entire kit instructions prior to use. Use only the materials supplied in this kit!

Always use proper PPE or refer to your organization's written protocol.

Humidity levels above 80% can slow results. Do not use in direct rain.

Device works best in temperatures between 38 and 90 degrees fahrenheit or 4 to 32 degrees celsius.

Maximum temperature range:
34 to 120 degrees fahrenheit
1 to 49 degrees celsius.


DO NOT open inner white pouch until you are ready to perform the evaluation.

Contact Us


Advnt Biotechnologies LLC USA
Toll free 888-223-3269
Emergency Information 24/7
602-803-1535

Technical information can also be found at www.advnt.org

Test Kit Equipment



Dropper/Swab Diluent tube



Pouched Test Device




Sim Card




Folded instruction insert


1

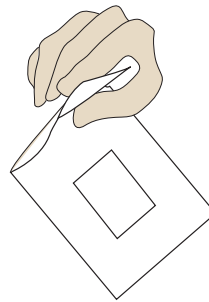


2

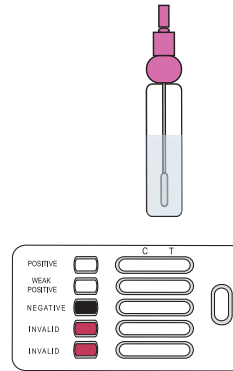


3

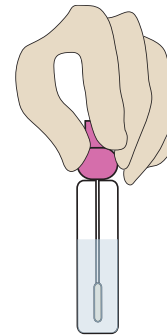

4

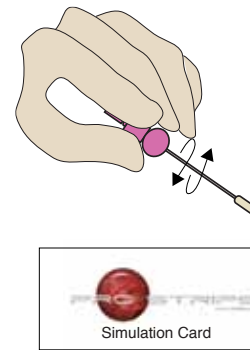

5



Tear open the inner white pouch to remove the test device. Place the device and the diluent tube on a flat, horizontal surface in front of you.

The test device should be placed in front of you with the text to your left as seen above.


Unscrew the cap from the diluent tube. While removing the swab, rub the foam tip against the inside walls to extract excess liquid then remove the swab completely.

Extract a test sample from the Pro Strips simulation card by swabbing the red portion of the logo for 5 seconds. Use a twirling motion to capture as much of the sample as possible. ThreatDust or ThreatJuice can also be used.

Return the swab back to the diluent tube and tighten the cap. Gently shake the tube for approximately 5 seconds.


MOVE TO STEP 6 ON THE BACK PAGE

6

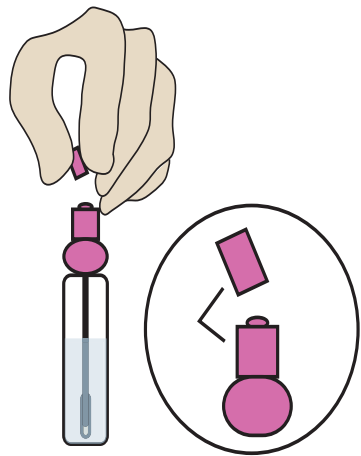

Remove the clear cap from the tip of the diluent tube. Break and remove the tip and discard. The tube now becomes a dropper for dispensing the sample onto the test device

7

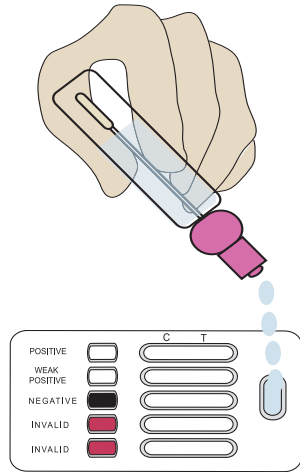


Invert the tube to a 45 degree angle and VERY SLOWLY add 10 to 11 drops to the sample well. DO NOT add more than 11 drops. Return the clear cap back to the dropper and set it to the side.

8




Set a timer and allow a maximum of 15 minutes before interpreting the results. You may see results in as little as 3 minutes. DO NOT interpret results after 30 minutes

9

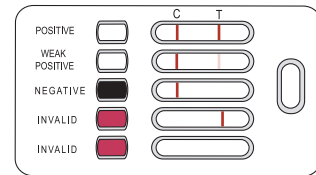


As the test begins to work, a reddish color will begin moving across the five (5) result windows. The last invalid window will not retain any color at the completion of the testing.

10

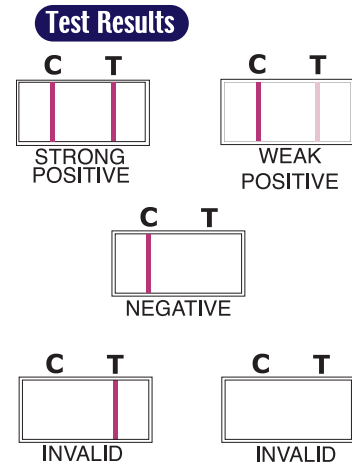

The windows above represent potential results. A weak positive, regardless of its intensity, should be considered positive. Invalids are rare but occur when tests are out-dated or exposed to extreme weather and should be re-run.

11

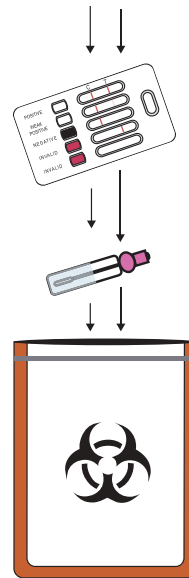

With your results collected, return all items back to the original foil pouch and zip lock shut. All items in this kit are non-toxic and can be safely disposed in the normal refuse.



Instruction Sheet

PS-5S

5

SIMULATION/TRAINER
PS-5S